

T C A T C G T A T C C A T C C C T A T C C A T C C C T  
C A T C C C T A T C G C T T C C A T C T G C T T C A  
T C T T C A T C C G T A T C T G C T T C C A T C T G C T  
C A T T T C A T C C G T A T C C A T C C A T C T G C T  
C T T C C A T C C C T A T C G C  
C A T C C A T C C C T A T C T G C T T C C A T C T G C T



**BIOTECON**

**Diagnostics**

# Product List

## - Kits & Reagents

Bacterial Pathogens

Viral Pathogens

Beverage Spoilage Organisms

Yeast and Mold

GMOs

Allergens

Animal Identification




Veterinary

Pharma

DNA/RNA Extraction

Additional Products

Valid from March 2017

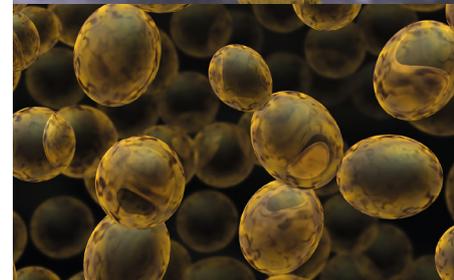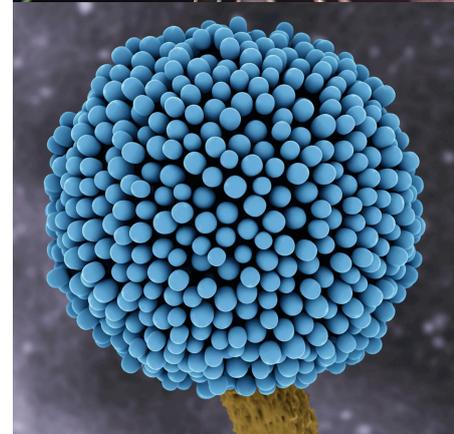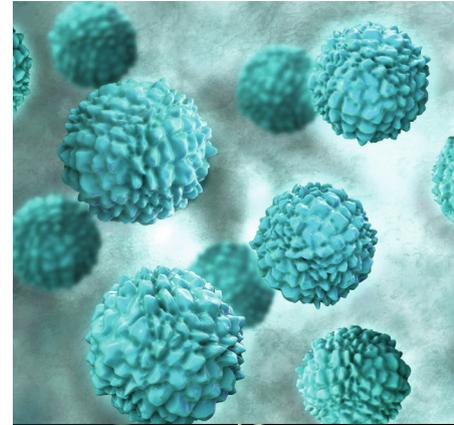

## Product List - Kits & Reagents

| order no.                  | real-time PCR Kits  | reactions | applicable to |        |                          |
|----------------------------|---|-----------|---------------|--------|--------------------------|
|                            |   |           | LC 2.0        | LC 480 | LC 96, PikoReal 24, etc* |
| <b>Bacterial Pathogens</b> |   |           |               |        |                          |
| <i>Salmonella</i>          |   |           |               |        |                          |
| R 602 27-1                 | foodproof® <i>Salmonella</i> Detection LyoKit - LP (AOAC-RI)                          | 96        | -             | +      | +                        |
| R 602 27-2                 | foodproof® <i>Salmonella</i> Detection LyoKit - RP (AOAC-RI)                          | 96        | -             | +      | +                        |
| R 602 27-1 L               | foodproof® <i>Salmonella</i> Detection LyoKit - LP (AOAC-RI)                          | 480       | -             | +      | +                        |
| R 602 27-2 L               | foodproof® <i>Salmonella</i> Detection LyoKit - RP (AOAC-RI)                          | 480       | -             | +      | +                        |
| R 302 27                   | foodproof® <i>Salmonella</i> Detection Kit (AOAC-RI + MicroVal + NordVal + DAFF)      | 96        | -             | +      | +                        |
| R 302 27 L                 | foodproof® <i>Salmonella</i> Detection Kit (AOAC-RI + MicroVal + NordVal + DAFF)      | 480       | -             | +      | +                        |
| R 310 27                   | foodproof® <i>Salmonella</i> Detection Kit (AOAC-RI + MicroVal + NordVal + DAFF)      | 96        | +             | +      | -                        |
| R 602 34-1                 | foodproof® <i>Salmonella</i> Enteritidis & Typhimurium Detection LyoKit - LP          | 96        | -             | +      | +                        |
| R 602 34-2                 | foodproof® <i>Salmonella</i> Enteritidis & Typhimurium Detection LyoKit - RP          | 96        | -             | +      | +                        |
| <i>Listeria</i>            |   |           |               |        |                          |
| R 602 20-1                 | foodproof® <i>Listeria</i> Genus Detection LyoKit - LP                                | 96        | -             | +      | +                        |
| R 602 20-2                 | foodproof® <i>Listeria</i> Genus Detection LyoKit - RP                                | 96        | -             | +      | +                        |
| R 302 20                   | foodproof® <i>Listeria</i> Genus Detection Kit  | 96        | -             | +      | +                        |
| R 300 20                   | foodproof® <i>Listeria</i> Genus Detection Kit  | 96        | +             | +      | -                        |
| R 602 23-1                 | foodproof® <i>Listeria monocytogenes</i> Detection LyoKit - LP (AOAC-RI)              | 96        | -             | +      | +                        |
| R 602 23-2                 | foodproof® <i>Listeria monocytogenes</i> Detection LyoKit - RP (AOAC-RI)              | 96        | -             | +      | +                        |
| R 302 23                   | foodproof® <i>Listeria monocytogenes</i> Detection Kit (AOAC-RI + NordVal)            | 96        | -             | +      | +                        |
| R 300 23                   | foodproof® <i>Listeria monocytogenes</i> Detection Kit (AOAC-RI + NordVal)            | 96        | +             | +      | -                        |
| <i>Escherichia coli</i>    |   |           |               |        |                          |
| R 302 10                   | foodproof® <i>E. coli</i> O157 Detection Kit (AOAC-RI)                                | 96        | -             | +      | +                        |
| R 300 10                   | foodproof® <i>E. coli</i> O157 Detection Kit (AOAC-RI)                                | 96        | +             | -      | -                        |
| R 300 09                   | foodproof® <i>E. coli</i> and <i>Shigella</i> Detection Kit                           | 96        | +             | +      | -                        |
| RDK 100 42-1               | foodproof® <i>E. coli</i> and <i>Shigella</i> LyoKit - LP                             | 96        | -             | +      | +                        |
| RDK 100 42-2               | foodproof® <i>E. coli</i> and <i>Shigella</i> LyoKit - RP                             | 96        | -             | +      | +                        |
| R 602 11-1                 | foodproof® STEC Screening LyoKit - LP (AOAC-RI pending)                               | 96        | -             | +      | +                        |
| R 602 11-2                 | foodproof® STEC Screening LyoKit - RP (AOAC-RI pending)                               | 96        | -             | +      | +                        |
| R 602 12-1                 | foodproof® STEC Identification LyoKit - LP (AOAC-RI pending)                          | 48        | -             | +      | +                        |
| R 602 12-2                 | foodproof® STEC Identification LyoKit - RP (AOAC-RI pending)                          | 48        | -             | +      | +                        |
| <i>Campylobacter</i>       |   |           |               |        |                          |
| R 302 05                   | foodproof® <i>Campylobacter</i> Quantification Kit                                    | 96        | -             | +      | +                        |
| R 310 05                   | foodproof® <i>Campylobacter</i> Detection Kit   | 96        | +             | +      | -                        |
| <i>Cronobacter</i>         |   |           |               |        |                          |
| R 302 15.1                 | foodproof® <i>Enterobacteriaceae</i> plus <i>Cronobacter</i> Detection Kit (MicroVal) | 96        | -             | +      | +                        |
| R 310 15.1                 | foodproof® <i>Enterobacteriaceae</i> plus <i>Cronobacter</i> Detection Kit (MicroVal) | 96        | +             | +      | -                        |
| R 310 15.1 L               | foodproof® <i>Enterobacteriaceae</i> plus <i>Cronobacter</i> Detection Kit (MicroVal) | 480       | +             | +      | -                        |
| R 602 13 -1                | foodproof® <i>Cronobacter</i> Detection LyoKit - LP                                   | 96        | -             | +      | +                        |
| R 602 13 -2                | foodproof® <i>Cronobacter</i> Detection LyoKit - RP                                   | 96        | -             | +      | +                        |

\* ABI 7500 (Fast), Biorad CFX96 and most other 5'Nuclease technology-based real-time PCR cyclers (please request)

Note: RDK = Pre-Launch Version, LP = Low Profile Microtiter Plate, RP = Regular Profile Microtiter Plate

foodproof®, microproof® and vetproof® are registered trademarks of BIOTECON Diagnostics. The above mentioned real-time PCR instruments are registered trademarks of their respective holders.

## Product List - Kits & Reagents

| order no.                          | real-time PCR Kits  | reactions | applicable to |        |                          |
|------------------------------------|---|-----------|---------------|--------|--------------------------|
|                                    |   |           | LC 2.0        | LC 480 | LC 96, PikoReal 24, etc* |
| <b>Vibrio</b>                      |   |           |               |        |                          |
| R 602 44-1                         | <b>foodproof®</b> <i>Vibrio</i> Detection LyoKit - LP (AOAC-RI pending)                 | 96        | -             | +      | +                        |
| R 602 44-2                         | <b>foodproof®</b> <i>Vibrio</i> Detection LyoKit - RP (AOAC-RI pending)                 | 96        | -             | +      | +                        |
| <b>Clostridium</b>                 |   |           |               |        |                          |
| R 602 40-1                         | <b>foodproof®</b> <i>Clostridium botulinum</i> Detection LyoKit - LP                    | 96        | -             | +      | +                        |
| R 602 40-2                         | <b>foodproof®</b> <i>Clostridium botulinum</i> Detection LyoKit - RP                    | 96        | -             | +      | +                        |
| RDK 100 23                         | <b>foodproof®</b> <i>Clostridium</i> Control Detection Kit                              | 64        | -             | +      | +                        |
| Z 700 08                           | <b>foodproof®</b> SL <i>Clostridium perfringens</i> Detection Kit                       | 50        | -             | +      | +                        |
| <b>Other Pathogens</b>             |   |           |               |        |                          |
| R 302 04                           | <b>foodproof®</b> <i>Brucella</i> Detection Kit   | 96        | -             | +      | +                        |
| RDK 100 11                         | <b>foodproof®</b> <i>Yersinia enterocolitica</i> Detection Kit                          | 96        | -             | +      | +                        |
| Z 700 05                           | <b>foodproof®</b> SL <i>Staphylococcus aureus</i> Detection Kit                         | 50        | -             | +      | +                        |
| Z 700 06                           | <b>foodproof®</b> SL <i>Bacillus cereus</i> Detection Kit                               | 50        | -             | +      | +                        |
| Z 700 09                           | <b>foodproof®</b> SL <i>Legionella pneumophila</i> Detection Kit                        | 50        | -             | +      | +                        |
| <b>Viral Pathogens</b>             |   |           |               |        |                          |
| RDK 100 32                         | <b>foodproof®</b> Hepatitis A Virus Detection Kit                                       | 64        | -             | +      | +                        |
| R 302 38.1                         | <b>foodproof®</b> Norovirus Detection Kit (GI, GII) (AOAC-RI pending)                   | 64        | -             | +      | +                        |
| RDK 100 35                         | <b>foodproof®</b> Norovirus (GI, GII) plus Hepatitis A Virus Detection Kit              | 64        | -             | +      | +                        |
| <b>Beverage Spoilage Organisms</b> |   |           |               |        |                          |
| R 602 02-1                         | <b>foodproof®</b> Beer Screening LyoKit - LP  | 96        | -             | +      | +                        |
| R 310 02                           | <b>foodproof®</b> Beer Screening Kit incl. <i>L. acetotolerans</i>                      | 96        | +             | +      | -                        |
| R 302 28                           | <b>foodproof®</b> <i>Alicyclobacillus</i> Detection Kit                                 | 96        | -             | +      | +                        |
| R 302 08                           | <b>foodproof®</b> <i>Dekkera</i> Quantification Kit                                     | 96        | -             | +      | +                        |
| R 300 26                           | <b>foodproof®</b> <i>Saccharomyces cerevisiae</i> var. <i>diastaticus</i> Detection Kit | 96        | -             | +      | +                        |
| RDK 100 37-1                       | <b>foodproof®</b> Spoilage Yeast Detection 1 LyoKit - LP                                | 96        | -             | +      | +                        |
| RDK 100 37-2                       | <b>foodproof®</b> Spoilage Yeast Detection 1 LyoKit - RP                                | 96        | -             | +      | +                        |
| RDK 100 38-1                       | <b>foodproof®</b> Spoilage Yeast Detection 2 LyoKit - LP                                | 96        | -             | +      | +                        |
| RDK 100 38-2                       | <b>foodproof®</b> Spoilage Yeast Detection 2 LyoKit - RP                                | 96        | -             | +      | +                        |
| <b>Yeast &amp; Mold</b>            |   |           |               |        |                          |
| R 602 42-1                         | <b>foodproof®</b> Yeast and Mold Quantification LyoKit - LP                             | 96        | -             | +      | +                        |
| R 602 42-2                         | <b>foodproof®</b> Yeast and Mold Quantification LyoKit - RP                             | 96        | -             | +      | +                        |

\* ABI 7500 (Fast), Biorad CFX96 and most other 5'Nuclease technology-based real-time PCR cyclers (please request)

Note: RDK = Pre-Launch Version, LP = Low Profile Microtiter Plate, RP = Regular Profile Microtiter Plate

**foodproof®**, **microproof®** and **vetproof®** are registered trademarks of BIOTECON Diagnostics. The above mentioned real-time PCR instruments are registered trademarks of their respective holders.

## Product List - Kits & Reagents

| order no.                           | real-time PCR Kits  | reactions | applicable to |        |                          |
|-------------------------------------|---|-----------|---------------|--------|--------------------------|
|                                     |   |           | LC 2.0        | LC 480 | LC 96, PikoReal 24, etc* |
| <b>GMOs</b>                         |   |           |               |        |                          |
| <b>GMO Screening</b>                |   |           |               |        |                          |
| R 602 17-1                          | foodproof® GMO Screening 1 LyoKit - LP (35S, NOS, FMV)  | 96        | -             | +      | +                        |
| R 602 17-2                          | foodproof® GMO Screening 1 LyoKit - RP (35S, NOS, FMV)  | 96        | -             | +      | +                        |
| R 602 18-1                          | foodproof® GMO Screening 2 LyoKit - LP (bar, P-35S-pat, CTP2-CP4-EPSPS, P-NOS-nptII, P-35S-nptII) | 96        | -             | +      | +                        |
| R 602 18-2                          | foodproof® GMO Screening 2 LyoKit - RP (bar, P-35S-pat, CTP2-CP4-EPSPS, P-NOS-nptII, P-35S-nptII) | 96        | -             | +      | +                        |
| R 302 17                            | foodproof® GMO Screening Kit (35S, NOS, bar, FMV), plant assay included                           | 128       | -             | +      | +                        |
| R 300 17                            | foodproof® GMO Screening Kit (35S, NOS), plant assay included                                     | 128       | +             | +      | -                        |
| R 602 21-1                          | foodproof® Plant Detection LyoKit - LP  | 96        | -             | +      | +                        |
| R 602 21-2                          | foodproof® Plant Detection LyoKit - RP  | 96        | -             | +      | +                        |
| <b>GMO Identification</b>           |   |           |               |        |                          |
| RDK 100 46                          | foodproof® GMO A5547-127 Soya Identification Kit  | 96        | -             | +      | +                        |
| RDK 100 47                          | foodproof® GMO MON87705 Soya Identification Kit   | 96        | -             | +      | +                        |
| RDK 100 48                          | foodproof® GMO FG72 Soya Identification Kit   | 96        | -             | +      | +                        |
| RDK 100 49                          | foodproof® GMO GMO DP356043 Soya Identification Kit   | 96        | -             | +      | +                        |
| Z 720 01                            | foodproof® SL GMO Bt11 Maize Detection Kit  | 50        | -             | +      | +                        |
| Z 720 02                            | foodproof® SL GMO GA21 Maize Detection Kit  | 50        | -             | +      | +                        |
| Z 720 03                            | foodproof® SL GMO MON810 Maize Detection Kit  | 50        | -             | +      | +                        |
| Z 720 04                            | foodproof® SL GMO T25 Maize Detection Kit   | 50        | -             | +      | +                        |
| Z 720 05                            | foodproof® SL GMO MIR162 Maize Detection Kit  | 50        | -             | +      | +                        |
| Z 720 06                            | foodproof® SL GMO MIR604 Maize Detection Kit  | 50        | -             | +      | +                        |
| Z 720 07                            | foodproof® SL GMO MON88017 Maize Detection Kit  | 50        | -             | +      | +                        |
| Z 720 08                            | foodproof® SL GMO MON89034 Maize Detection Kit  | 50        | -             | +      | +                        |
| Z 720 09                            | foodproof® SL GMO NK603 Maize Detection Kit   | 50        | -             | +      | +                        |
| Z 720 10                            | foodproof® SL GMO TC1507 Maize Detection Kit  | 50        | -             | +      | +                        |
| Z 720 11                            | foodproof® SL GMO DAS59112-7 Maize Detection Kit  | 50        | -             | +      | +                        |
| Z 720 12                            | foodproof® SL GMO MON863 Maize Detection Kit  | 50        | -             | +      | +                        |
| Z 722 01                            | foodproof® SL GMO A2704-12 Soya Detection Kit   | 50        | -             | +      | +                        |
| Z 722 02                            | foodproof® SL GMO GTS40-3-2 Soya Detection Kit  | 50        | -             | +      | +                        |
| <b>GMO Multiplex Identification</b> |   |           |               |        |                          |
| RDK 100 29                          | foodproof® GMO Soya Identification 1 LyoKit (DAS-44406-6, MON87701, MON87708, MON87769)           | 96        | -             | +      | +                        |
| RDK 100 30                          | foodproof® GMO Soya Identification 2 LyoKit (BPS-CV127-9, DP-305423-1, DAS-68416-4, DAS-81419-2)  | 96        | -             | +      | +                        |
| RDK 100 36                          | foodproof® GMO Maize Identification 1 LyoKit (DAS-40278-9, LY038, VCO-01981-5)                    | 96        | -             | +      | +                        |
| Z 725 01                            | foodproof® SL GMO Maize Multiplex Detection Kit (GA21, MIR604)                                    | 50        | -             | +      | +                        |
| Z 725 02                            | foodproof® SL GMO Maize Multiplex Detection Kit (MON89034, CBH351, Bt176)                         | 50        | -             | +      | +                        |
| Z 725 03                            | foodproof® SL GMO Maize Multiplex Detection Kit (MON88017, NK603, MIR162)                         | 50        | -             | +      | +                        |
| Z 725 06                            | foodproof® SL GMO Maize Multiplex Detection Kit (Bt11, TC1507)                                    | 50        | -             | +      | +                        |
| Z 725 07                            | foodproof® SL GMO Maize Multiplex Detection Kit (T25, MON810, MON863)                             | 50        | -             | +      | +                        |
| <b>GMO Quantification</b>           |   |           |               |        |                          |
| R 302 29                            | foodproof® GMO 35S Maize Quantification Kit   | 128       | -             | +      | +                        |
| R 302 16                            | foodproof® GMO Bt176 Maize Quantification Kit   | 128       | +             | +      | +                        |
| R 302 19                            | foodproof® GMO RR Soya Quantification Kit   | 128       | -             | +      | +                        |
| R 300 19                            | foodproof® GMO RR Soya Quantification Kit   | 128       | +             | +      | -                        |
| R 302 35                            | foodproof® GMO RR 2 Yield Soya Quantification Kit   | 128       | -             | +      | +                        |

\* ABI 7500 (Fast), Biorad CFX96 and most other 5'Nuclease technology-based real-time PCR cyclers (please request)

Note: RDK = Pre-Launch Version, LP = Low Profile Microtiter Plate, RP = Regular Profile Microtiter Plate

foodproof®, microproof® and vetproof® are registered trademarks of BIOTECON Diagnostics. The above mentioned real-time PCR instruments are registered trademarks of their respective holders.

## Product List - Kits & Reagents

| order no.                    | real-time PCR Kits   | reactions                                 | applicable to |        |                          |
|------------------------------|--|---|---------------|--------|--------------------------|
|                              |  |   | LC 2.0        | LC 480 | LC 96, PikoReal 24, etc* |
| <b>Allergens</b>             |  |   |               |        |                          |
| R 302 60                     | <b>foodproof®</b> Celery Detection Kit   | 64  | -             | +      | +                        |
| R 302 61                     | <b>foodproof®</b> Soya Detection Kit   | 64  | -             | +      | +                        |
| R 302 62                     | <b>foodproof®</b> Hazelnut Detection Kit   | 64  | -             | +      | +                        |
| R 302 63                     | <b>foodproof®</b> Peanut Detection Kit   | 64  | -             | +      | +                        |
| R 302 64                     | <b>foodproof®</b> Gluten Detection Kit   | 64  | -             | +      | +                        |
| <b>Animal Identification</b> |  |   |               |        |                          |
| R 602 43-1                   | <b>foodproof®</b> Porcine Detection LyoKit - LP  | 96  | -             | +      | +                        |
| R 602 43-2                   | <b>foodproof®</b> Porcine Detection LyoKit - RP  | 96  | -             | +      | +                        |
| RDK 100 39-1                 | <b>foodproof®</b> Animal Detection 1 LyoKit (Porcine, Bovine, Equine) - LP                                       | 96  | -             | +      | +                        |
| RDK 100 39-2                 | <b>foodproof®</b> Animal Detection 1 LyoKit (Porcine, Bovine, Equine) - RP                                       | 96  | -             | +      | +                        |
| RDK 100 07                   | <b>foodproof®</b> Donkey Detection Kit   | 96  | -             | +      | +                        |
| Z 730 01                     | <b>foodproof®</b> SL Porcine Species Detection Kit   | 50  | -             | +      | +                        |
| Z 730 02                     | <b>foodproof®</b> SL Bovine Species Detection Kit  | 50  | -             | +      | +                        |
| Z 730 03                     | <b>foodproof®</b> SL Sheep Species Detection Kit   | 50  | -             | +      | +                        |
| Z 730 04                     | <b>foodproof®</b> SL Horse Species Detection Kit   | 50  | -             | +      | +                        |
| Z 730 05                     | <b>foodproof®</b> SL Chicken Species Detection Kit   | 50  | -             | +      | +                        |
| Z 730 06                     | <b>foodproof®</b> SL Goat Species Detection Kit  | 50  | -             | +      | +                        |
| Z 730 07                     | <b>foodproof®</b> SL Duck Species Detection Kit  | 50  | -             | +      | +                        |
| Z 730 08                     | <b>foodproof®</b> SL Shrimp and Crab Species Detection Kit   | 50  | -             | +      | +                        |
| <b>Veterinary</b>            |  |   |               |        |                          |
| V 900 01                     | <b>vetproof®</b> SE Vaccine Detection 1 Kit**  | 48  | -             | +      | +                        |
| V 900 27                     | <b>vetproof®</b> <i>Salmonella</i> Detection Kit**   | 96  | -             | +      | +                        |
| Z 740 01                     | <b>vetproof®</b> SL <i>Mycoplasma</i> Multiplex Detection Kit ( <i>M. gallisepticum</i> , <i>M. synoviae</i> )** | 50  | -             | +      | +                        |
| <b>Pharma</b>                |  |   |               |        |                          |
| R 300 31                     | <b>microproof®</b> Hygiene Screening System  | 96  | +             | +      | -                        |
| R 300 32                     | <b>microproof®</b> <i>Streptococcus pneumoniae</i> Detection Kit   | 96  | +             | +      | -                        |
| <b>Additional Products</b>   |  |   |               |        |                          |
| Color Compensation Kits      |  | runs                                      |               |        |                          |
| A 500 08                     | Color Compensation Set 1   | 5   | -             | +      | -                        |
| A 500 10                     | Color Compensation Set 3   | 5   | -             | +      | -                        |
| A 500 11                     | Color Compensation Set 4   | 5   | +             | -      | -                        |
| A 500 15                     | Color Compensation Set 5   | 5   | -             | +      | -                        |
| Other                        |  | applicable to                             |               |        |                          |
| A 500 13                     | Allergen RM 800 Reference Material   | <b>foodproof®</b> Allergen Detection Kits |               |        |                          |

\* ABI 7500 (Fast), Biorad CFX96 and most other 5'Nuclease technology-based real-time PCR cyclers (please request)

\*\* Regulatory requirements vary by country; products may not be available in your geographic area

Note: RDK = Pre-Launch Version, LP = Low Profile Microtiter Plate, RP = Regular Profile Microtiter Plate

**foodproof®**, **microproof®** and **vetproof®** are registered trademarks of BIOTECON Diagnostics. The above mentioned real-time PCR instruments are registered trademarks of their respective holders.

## Product List - Kits & Reagents

| order no. | DNA/RNA Extraction Kits | isolations | applicable to |
|-----------|-------------------------|------------|---------------|
|-----------|-------------------------|------------|---------------|

### StarPrep

|            |   |     |   |
|------------|---|-----|---|
| S 400 07   | <b>foodproof®</b> StarPrep One Kit (AOAC, MicroVal) | 100 | <i>Enterobacteriaceae, Salmonella, Cronobacter, E. coli, Shigella</i> |
| S 400 07 L | <b>foodproof®</b> StarPrep One Kit (AOAC, MicroVal) | 500 | <i>Enterobacteriaceae, Salmonella, Cronobacter, E. coli, Shigella</i> |
| S 400 08   | <b>foodproof®</b> StarPrep Two Kit                  | 96  | <i>Listeria, Campylobacter, Alicyclobacillus, Yeast &amp; Mold</i>    |
| S 400 17 L | <b>foodproof®</b> StarPrep Two 8-Strip Kit          | 480 | <i>Listeria</i>   |
| S 400 18   | <b>foodproof®</b> StarPrep Three Kit                | 96  | Beer, <i>Vibrio</i> , STEC  |
| S 400 09   | <b>foodproof®</b> StarPrep Four Kit                 | 96  | Yeast   |

### ShortPrep

|          |  |    |   |
|----------|--|----|---|
| S 400 01 | <b>foodproof®</b> ShortPrep I Kit (AOAC, NordVal)  | 96 | <i>Salmonella</i>                                 |
| S 400 02 | <b>foodproof®</b> ShortPrep II Kit (AOAC, NordVal) | 96 | <i>Listeria, Campylobacter, E. coli, Shigella</i> |

### Sample Preparation

|            |  |     |   |
|------------|--|-----|---|
| S 400 04   | <b>foodproof®</b> Sample Preparation Kit I   | 100 | <i>Enterobacteriaceae, Salmonella, Cronobacter, E. coli, Shigella</i> |
| S 400 05   | <b>foodproof®</b> Sample Preparation Kit II  | 100 | <i>Listeria, Campylobacter, Alicyclobacillus</i>                      |
| S 400 06.1 | <b>foodproof®</b> Sample Preparation Kit III | 50  | GMOs, Allergens and Animal ID   |
| S 400 16   | <b>foodproof®</b> Sample Preparation Kit IV  | 50  | Viruses   |

### Magnetic Preparation

|            |   |     |  |
|------------|---|-----|--|
| S 400 11   | <b>foodproof®</b> Magnetic Preparation Kit I (AOAC, MicroVal) | 96  | <i>Salmonella, Cronobacter, E. coli, Shigella</i>  |
| S 400 11 L | <b>foodproof®</b> Magnetic Preparation Kit I (AOAC, MicroVal) | 480 | <i>Salmonella, Cronobacter, E. coli, Shigella</i>  |
| S 400 12 L | <b>foodproof®</b> Magnetic Preparation Kit II                 | 480 | <i>Listeria</i>                                    |
| S 400 13 L | <b>foodproof®</b> Magnetic Preparation Kit III                | 480 | GMOs, Allergens and Animal ID                      |
| S 400 15 L | <b>foodproof®</b> Magnetic Preparation Kit IV                 | 480 | <i>Enterobacteriaceae, Salmonella, Cronobacter</i> |
| S 400 19 L | <b>foodproof®</b> Magnetic Preparation Kit V                  | 480 | <i>Salmonella</i> in PPS samples                   |
| RDK 100 43 | <b>foodproof®</b> Magnetic Preparation Kit VI                 | 480 | Veterinary Viruses                                 |

### Additional Products

| Reagents   | applicable to  |
|--|--|
| A 500 02 S Reagent D, 15 ml (MicroVal)               | <b>foodproof®</b> <i>Vibrio</i> Detection LyoKit   |
| A 500 02 Reagent D, 30 ml (MicroVal)                 | <b>foodproof®</b> <i>Enterobacteriaceae</i> plus <i>Cronobacter</i> Detection Kit, <b>foodproof®</b> Yeast and Mold Quantification LyoKit, <b>foodproof®</b> Spoilage Yeast Detection 1 LyoKit |
| A 500 02 L Reagent D, 150 ml (MicroVal)              | <b>foodproof®</b> <i>Enterobacteriaceae</i> plus <i>Cronobacter</i> Detection Kit  |
| A 500 12 Reagent P                                   | <b>foodproof®</b> Magnetic Preparation Kit I (protein-rich samples)  |
| A 500 14 Resuspension Reagent                        | <b>foodproof®</b> Star Prep Two Kit  |
| Z 800 01 <b>foodproof®</b> <i>Listeria</i> StarBroth | <b>foodproof®</b> <i>Listeria monocytogenes</i> Detection LyoKit, <b>foodproof®</b> <i>Listeria</i> Genus Detection (Lyo)Kit   |